


Time Deviation $\sigma_x(\tau)$

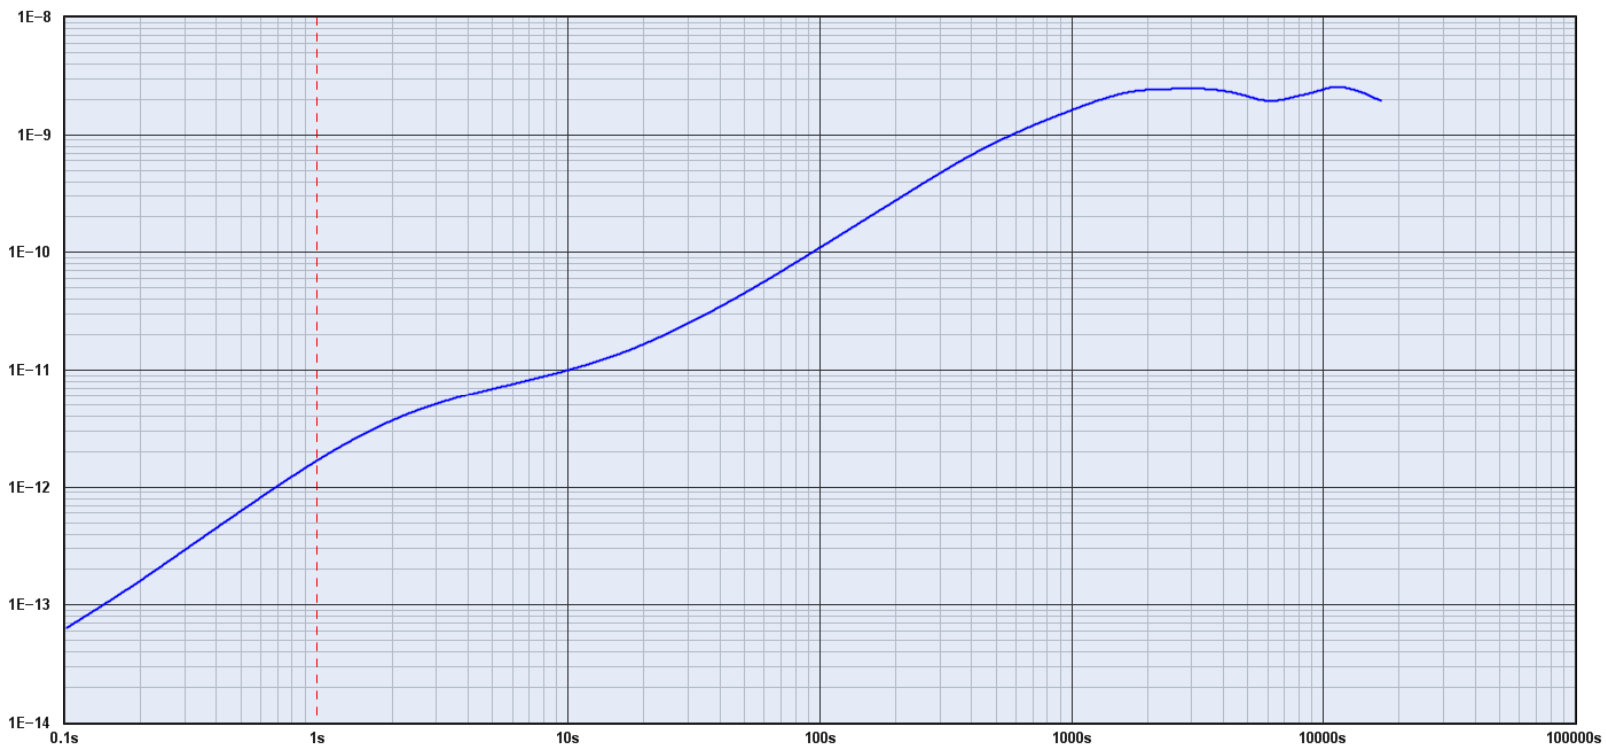

Trace	Notes	Input Freq	Sample Interval	TDEV at 1s	Duration	Acquired	Instrument
15M vs Cs		15 MHz	0.100 s	$1.72E-12$	1d 0h 0m 0s	864000 pts	TimePod 5330A